



# Microplate, 384-well 781980

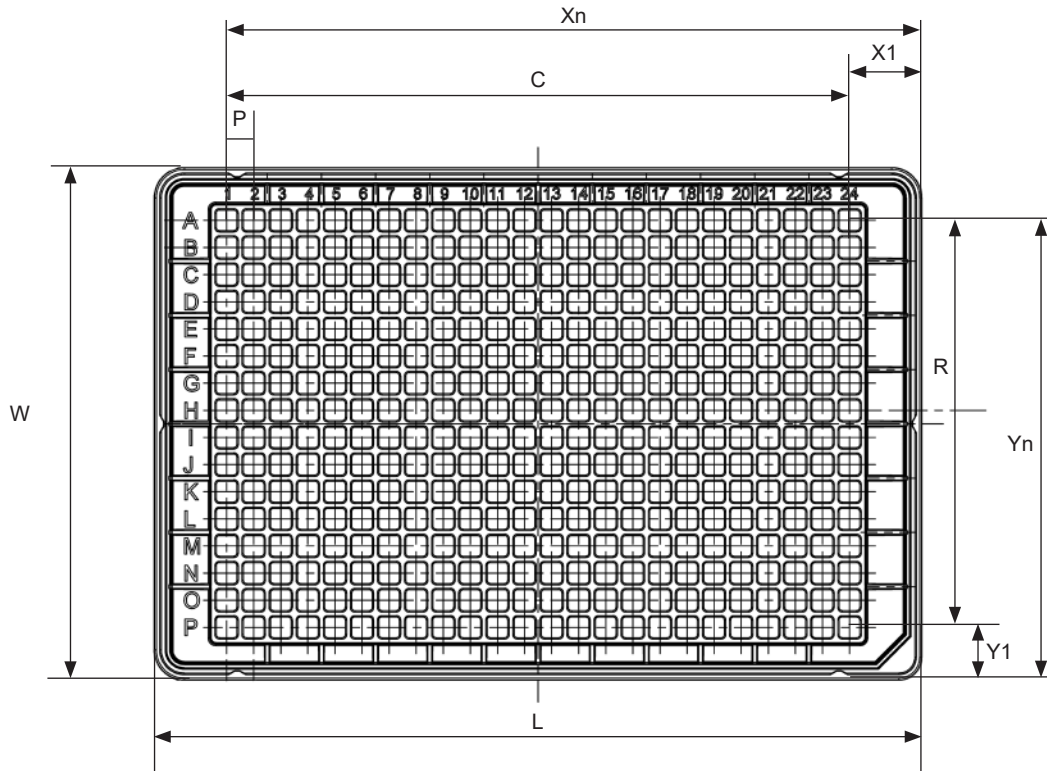

L	127.76 mm
W	85.45 mm
H	11.50 mm
Hs	3.50 mm
X1	12.03 mm
Xn	115.53 mm
Y1	8.78 mm
Yn	76.28 mm
P	4.50 mm
D	3.90 mm
Hw	8.85 mm
C	24 Well
R	16 Well

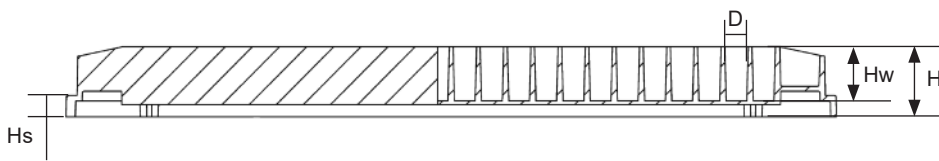


<b>Type</b>	standard
<b>Base shape</b>	F-bottom
<b>Surface</b>	cellGrade™
<b>Volume</b>	100 µl / well
<b>Material</b>	PS
<b>Color</b>	transparent
<b>Quality</b>	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




\* human and bacterial DNA, \*\* according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

# Microplate, 384-well 781981

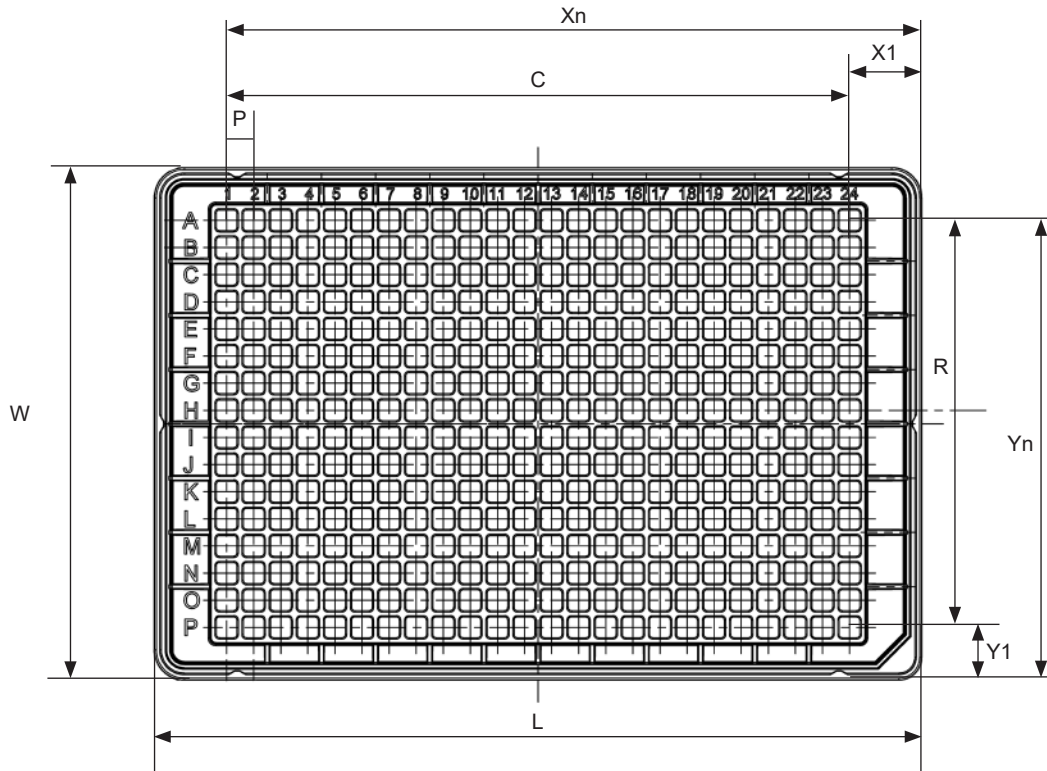

L	127.76 mm
W	85.45 mm
H	11.50 mm
Hs	3.50 mm
X1	12.03 mm
Xn	115.53 mm
Y1	8.78 mm
Yn	76.28 mm
P	4.50 mm
D	3.90 mm
Hw	8.85 mm
C	24 Well
R	16 Well

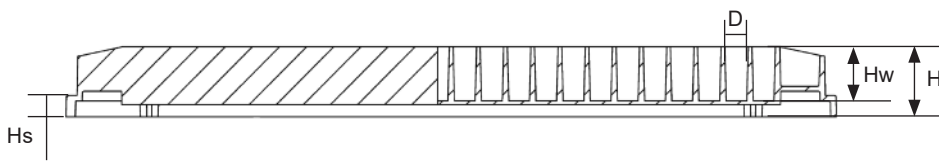


Type	standard
Base shape	F-bottom
Surface	cellGrade™
Volume	100 µl / well
Material	PS
Color	white
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




\* human and bacterial DNA, \*\* according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

# Microplate, 384-well 781982

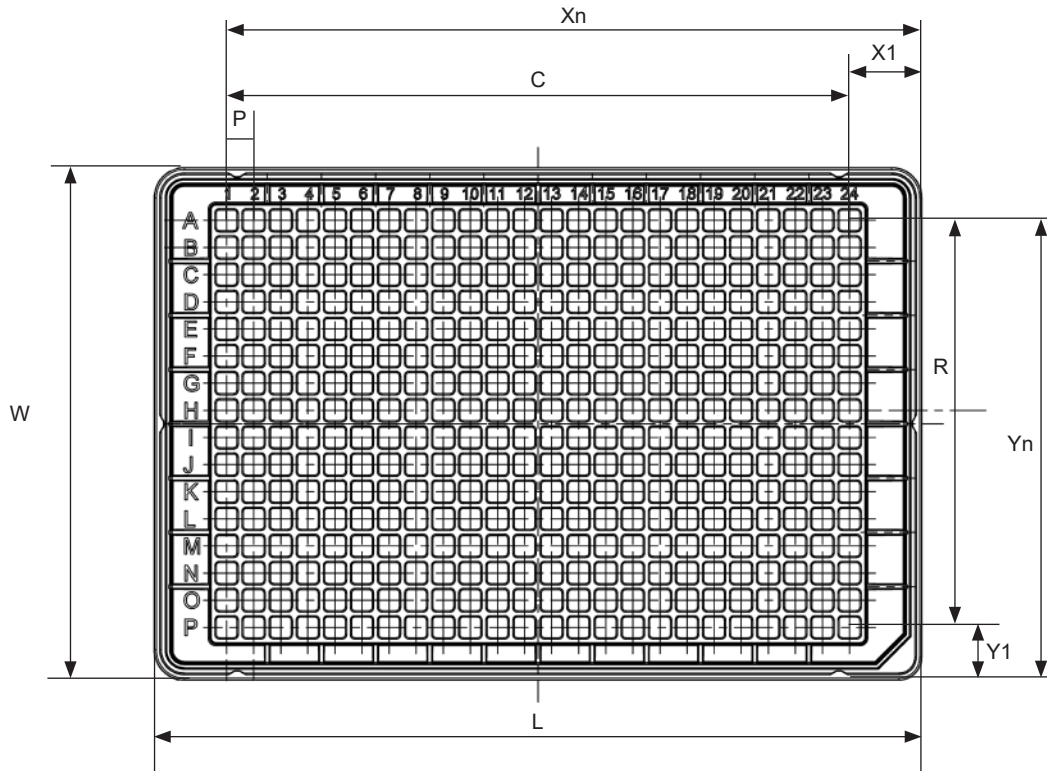

L	127.76 mm
W	85.45 mm
H	11.50 mm
Hs	3.50 mm
X1	12.03 mm
Xn	115.53 mm
Y1	8.78 mm
Yn	76.28 mm
P	4.50 mm
D	3.90 mm
Hw	8.85 mm
C	24 Well
R	16 Well

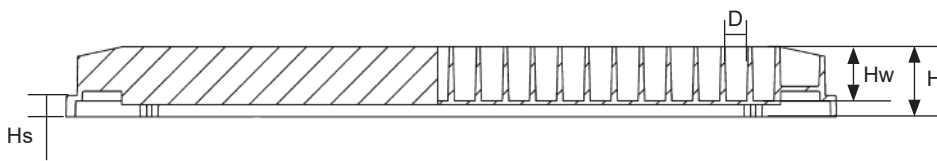

<b>Type</b>	standard
<b>Base shape</b>	F-bottom
<b>Surface</b>	cellGrade™
<b>Volume</b>	100 µl / well
<b>Material</b>	PS
<b>Color</b>	black
<b>Quality</b>	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




\* human and bacterial DNA, \*\* according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

# Microplate, 384-well

## 781986 | 781988

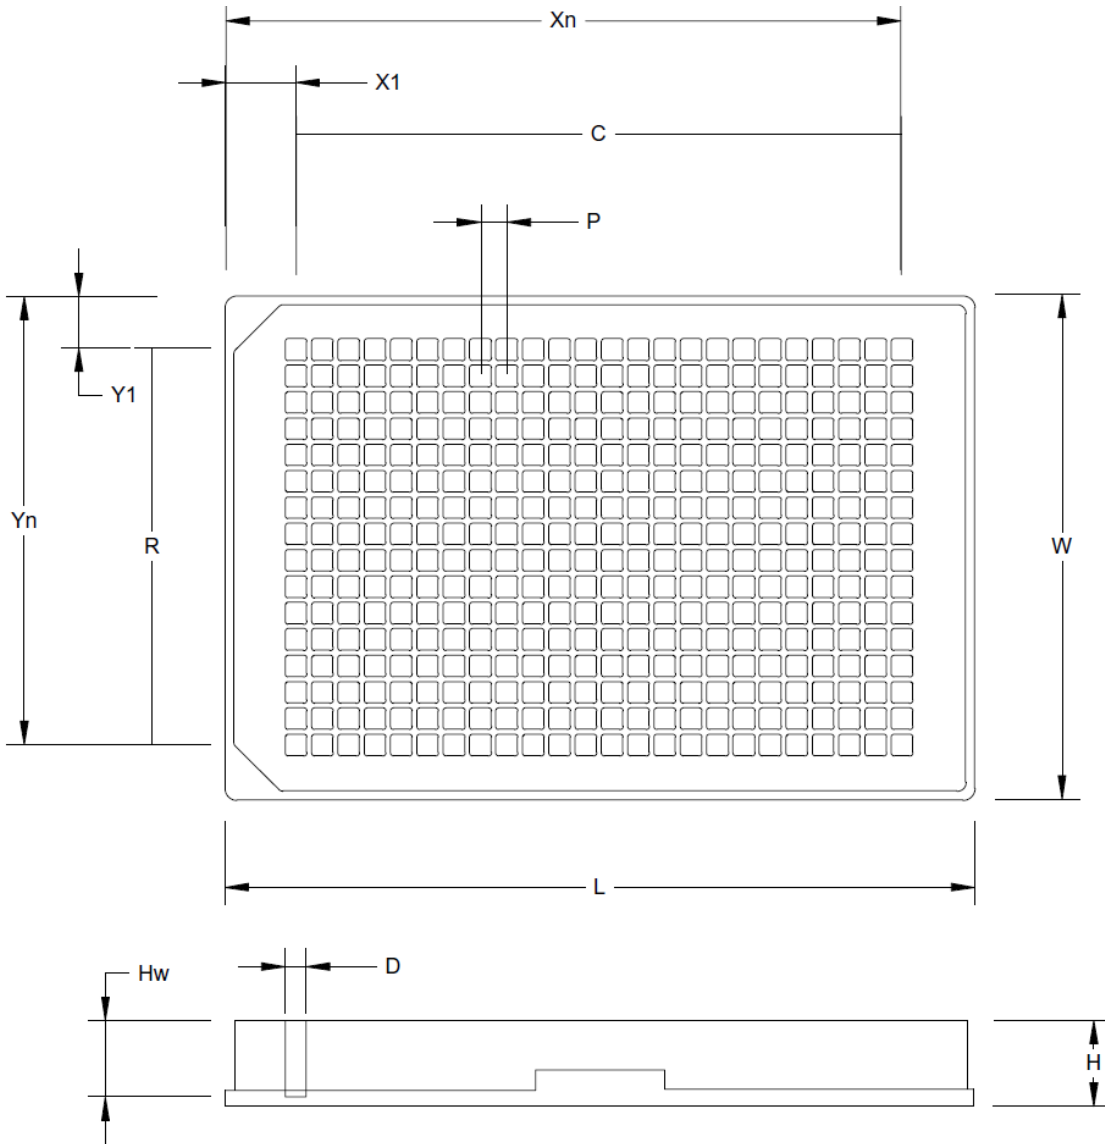

L	127.60 mm
W	85.60 mm
H	14.80 mm
Hs	2.75 mm
X1	12.10 mm
Xn	115.60 mm
Y1	9.10 mm
Yn	76.60 mm
P	4.50 mm
D	3.65 mm
Hw	11.95 mm
C	24 Well
R	16 Well

<b>Type</b>	standard, transparent bottom
<b>Base shape</b>	F-bottom
<b>Surface</b>	cellGrade™
<b>Volume</b>	120 µl / well
<b>Material</b>	PS
<b>Color</b>	white
<b>Quality</b>	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




\* human and bacterial DNA, \*\* according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

# Microplate, 384-well

## 781987 | 781989

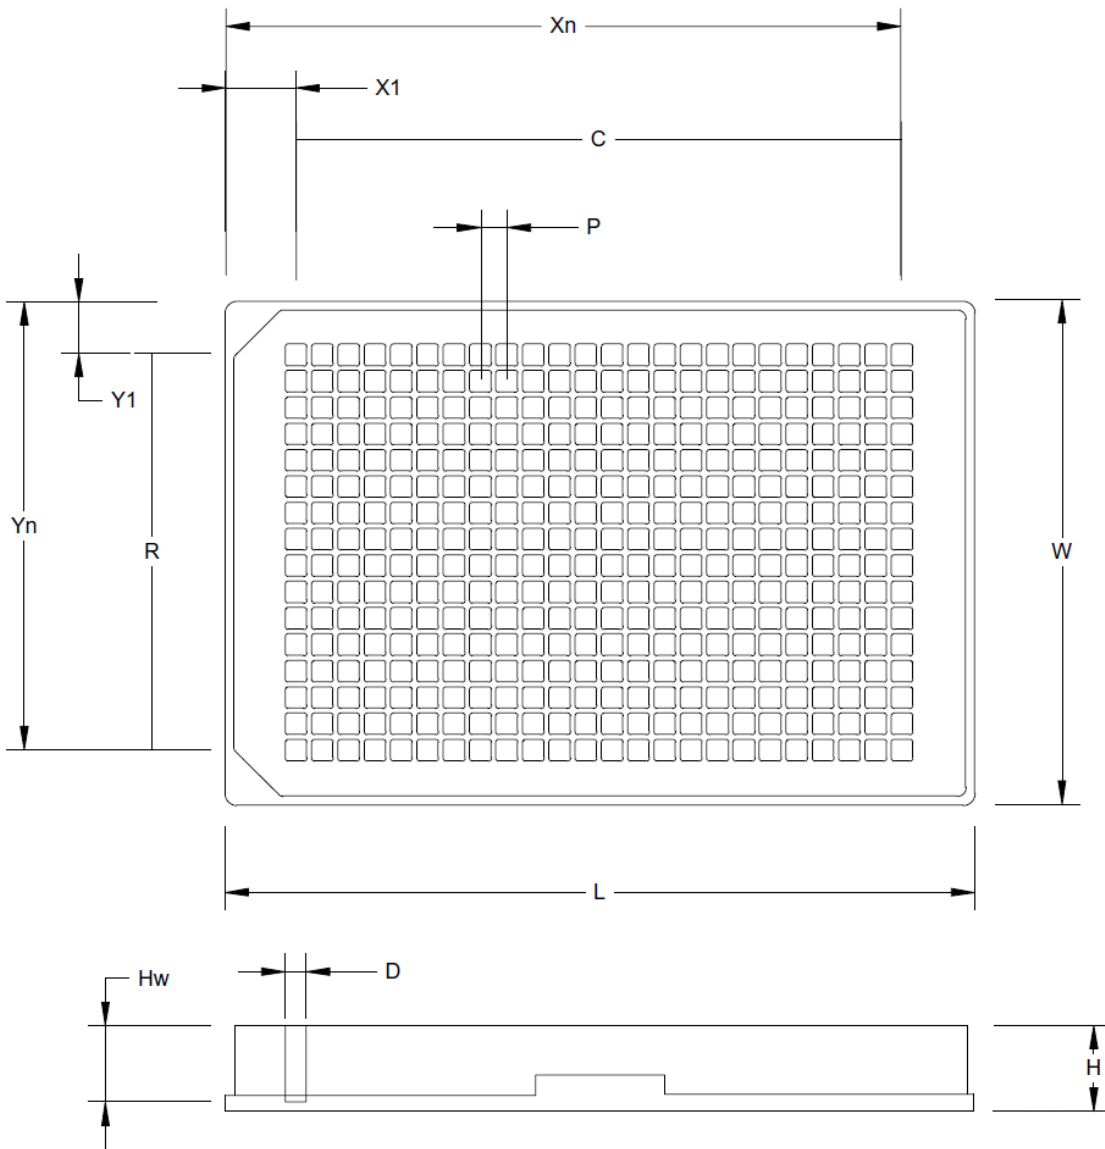

L	127.60 mm
W	85.60 mm
H	14.80 mm
Hs	2.75 mm
X1	12.10 mm
Xn	115.60 mm
Y1	9.10 mm
Yn	76.60 mm
P	4.50 mm
D	3.65 mm
Hw	11.95 mm
C	24 Well
R	16 Well

<b>Type</b>	standard, transparent bottom
<b>Base shape</b>	F-bottom
<b>Surface</b>	cellGrade™
<b>Volume</b>	120 µl / well
<b>Material</b>	PS
<b>Color</b>	black
<b>Quality</b>	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5



\* human and bacterial DNA, \*\* according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.