


BRANDplates® multi-well plates, for inserts, 24-well 782880

PRODUCT
INFORMATION



Type	standard
Surface	pureGrade™ S
Volume	1,5 - 2 ml / well
Material	PS
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5

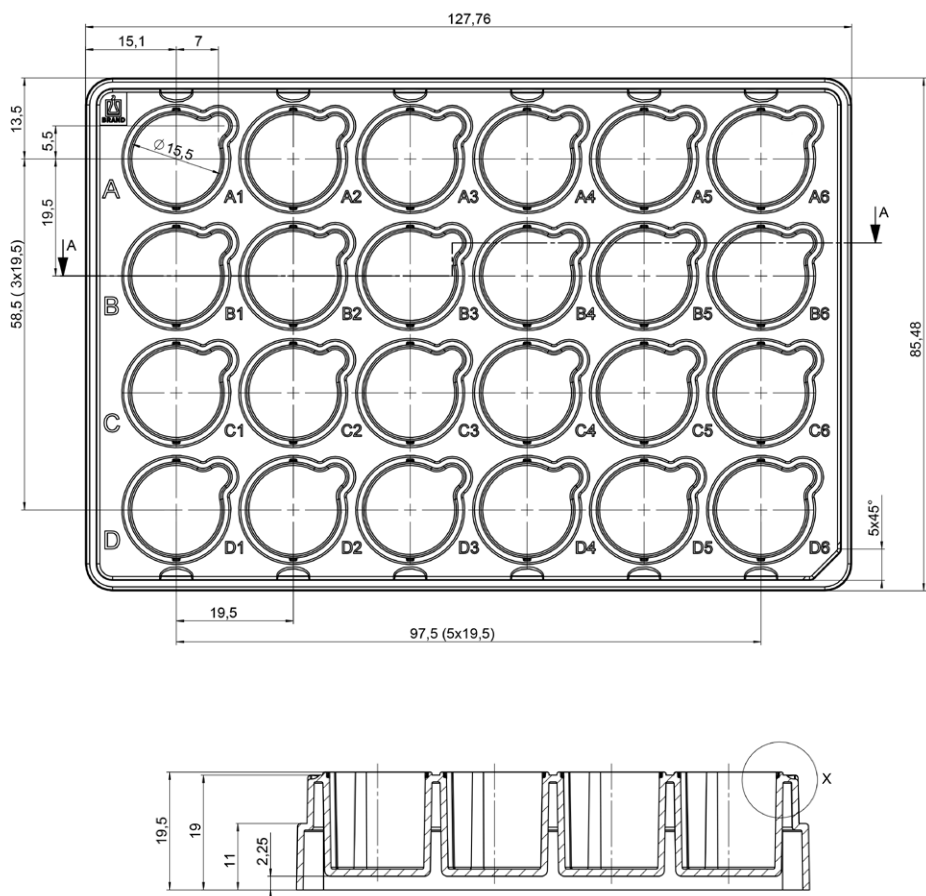


* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml


Subject to technical modification without notice. Errors excepted.

BRANDplates® multi-well plates, for inserts, 6-well 782881

PRODUCT
INFORMATION

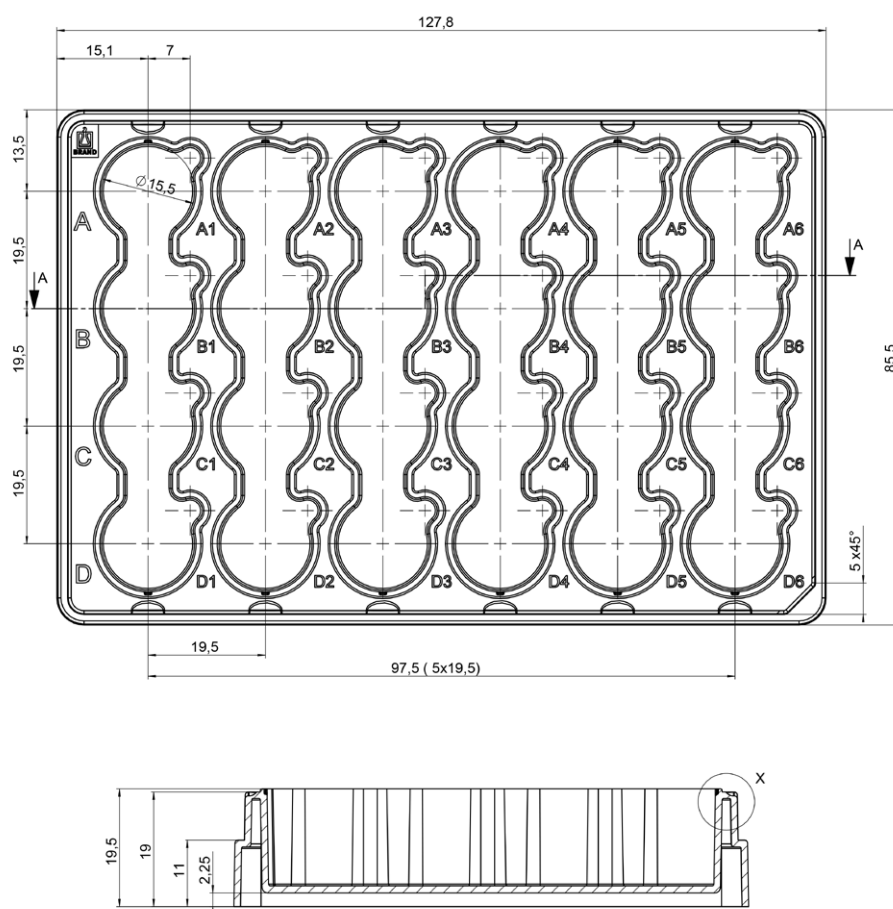

Type	standard
Surface	pureGrade™ S
Volume	8 - 10 ml / well
Material	PS
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

BRANDplates® multi-well plates, for inserts, 24-well 782890

PRODUCT
INFORMATION

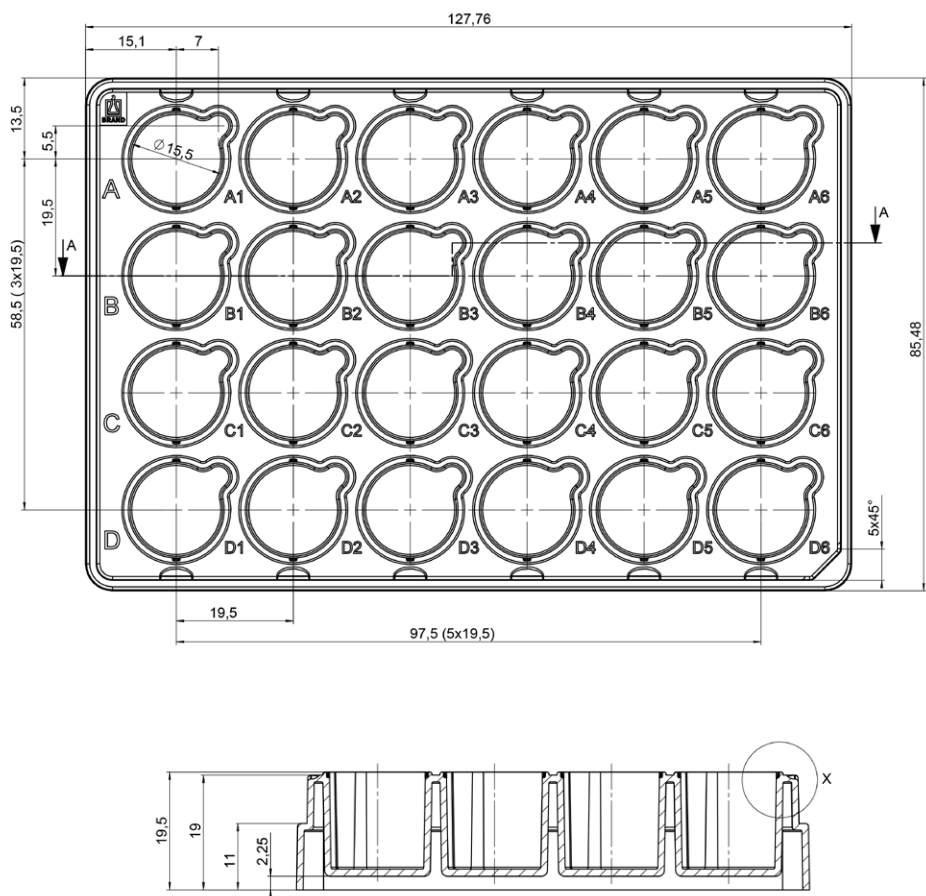

Type	standard
Surface	cellGrade™ plus
Volume	1,5 - 2 ml / well
Material	PS
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5




* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.

BRANDplates® multi-well plates, for inserts, 6-well 782891

PRODUCT
INFORMATION

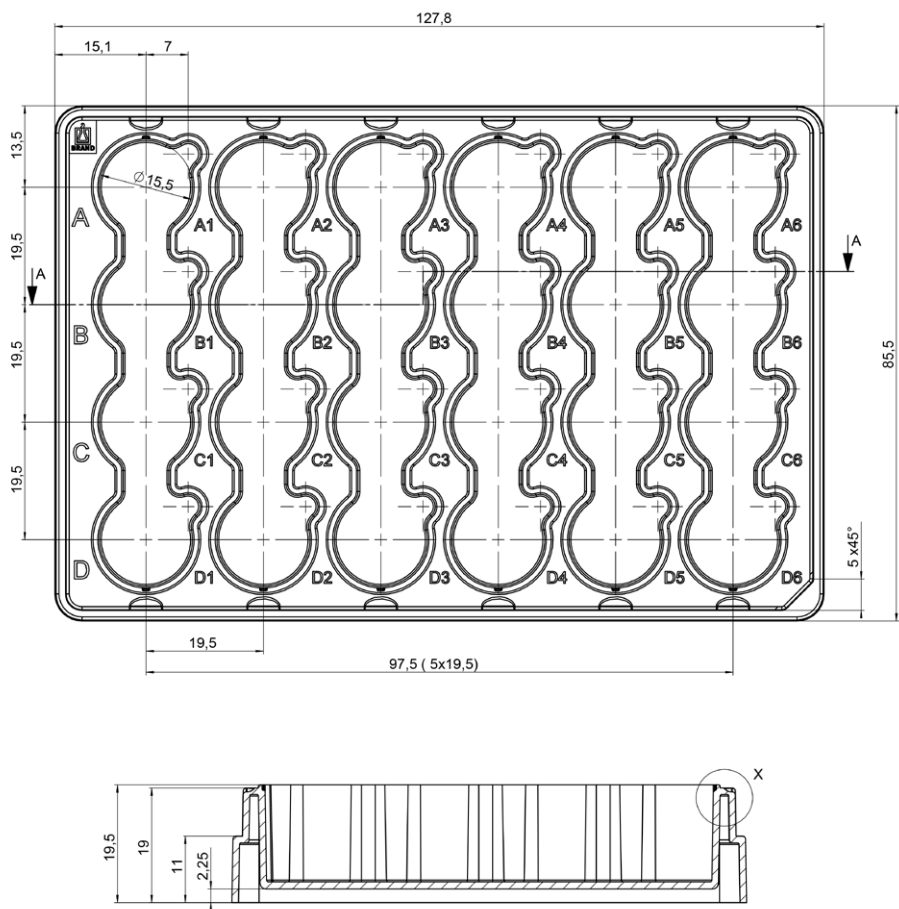

Type	standard
Surface	cellGrade™ plus
Volume	8 - 10 ml / well
Material	PS
Color	transparent
Quality	Cleanroom class 8 according to ISO 14 644-1, Free of DNA*, RNase and DNase, Free of pyrogens, according to LAL test **, Sterile according to ISO 11 137, Free of cytotoxic substances acc. ISO 10 993-5



* human and bacterial DNA, ** according to Limulus Amebocyte Lysate (LAL) test, detection limit 0.01 EU/ml

Subject to technical modification without notice. Errors excepted.